


Reprocessing of Rigid Endoscopes

Pre-Clean, Patient Care Area



- ▣ Pre-clean scope before transport to CSSD

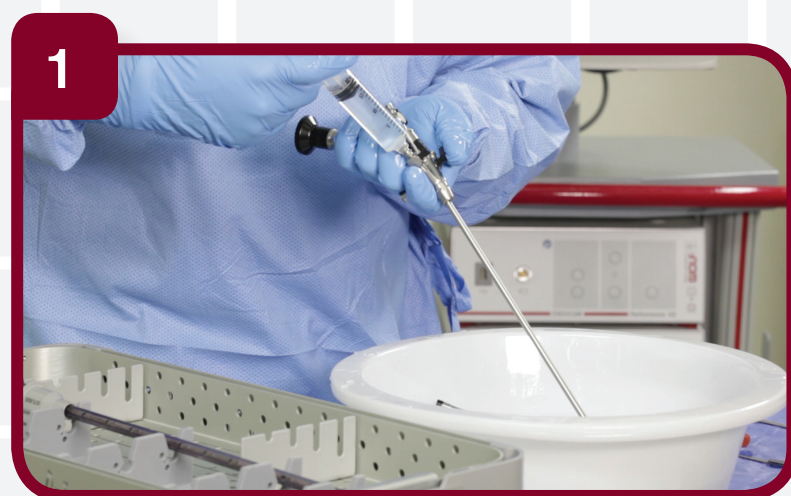

- ▣ Use manual cleaning or pre-treat spray



- ▣ Attach scope protector before transport
- ▣ Secure in tray or transport bin to prevent damage
- ▣ Transport to CSSD as soon as possible