

Rigid endoscopes with channel by Richard Wolf

1



2




3



Pre-cleaning


4

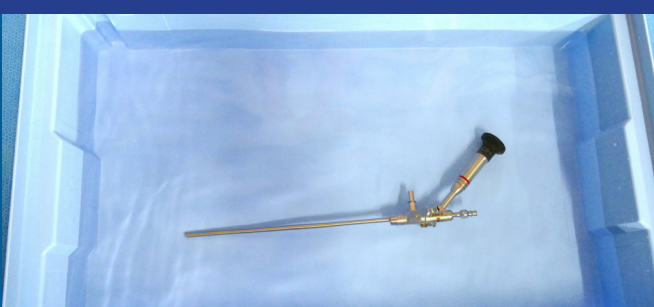

5




6

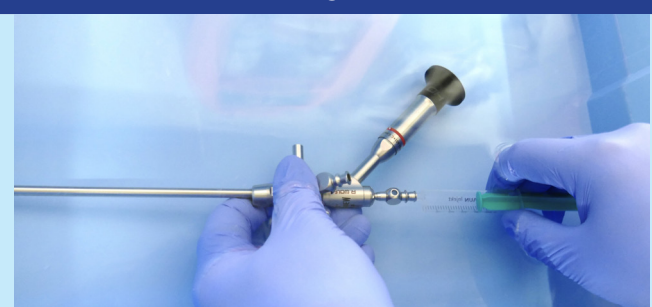

—



Manual disinfection

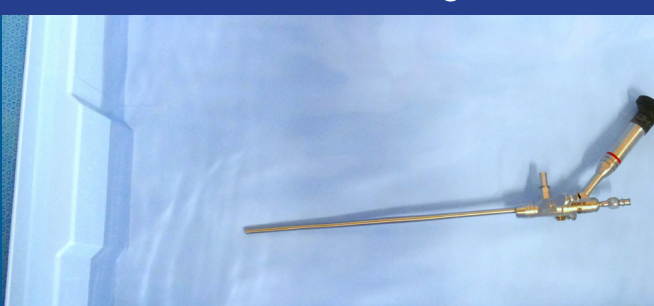


9



10



Manual drying

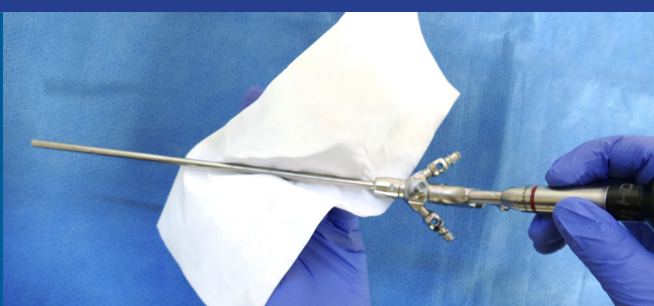

12



13



Functional testing, maintenance

Sterilization and storage



15



16



17



Storage of sterilized medical devices according to ISO 11607 – taking into account the applicable national requirements.



This Quick Guide is an overview. It does not replace the specific instructions for use of the respective flexible endoscope. The respective instructions for use must be observed. This Quick Guide can only be used as a supplement to the instructions for use.